National Defence / Défense nationale

UNCLASSIFIED

UNLIMITED DISTRIBUTION

DRES

SUFFIELD MEMORANDUM

NO. 1104

AN INVESTIGATION OF THE SUITABILITY OF USING A SIEGLAFF-MCKELVEY HIGH SHEAR RATE MELT RHEOMETER FOR THE MEASUREMENT OF LOW VISCOSITY POLYMER SOLUTIONS (U)

by

J.B. Hacker*

PCN No. 13E10

August 1984

* Co-operative student from the University of British Columbia, May — August 1983

DEFENCE RESEARCH ESTABLISHMENT SUFFIELD : RALSTON : ALBERTA

Canada

WARNING
The use of this information is permitted subject to recognition of proprietary and patent rights.

UNCLASSIFIED

UNLIMITED
DISTRIBUTION

DEFENCE RESEARCH ESTABLISHMENT SUFFIELD
RALSTON ALBERTA

SUFFIELD MEMORANDUM NO. 1104

AN INVESTIGATION OF THE SUITABILITY OF USING A SIEGLAFF-MCKELVEY HIGH SHEAR RATE MELT RHEOMETER FOR THE MEASUREMENT OF LOW VISCOSITY POLYMER SOLUTIONS (U)

by

J.B. Hacker*

PCN No. 13E10

WARNING
The use of this information is permitted subject to recognition of proprietary and patent rights".

* Co-operative student from the University of British Columbia, May — August 1983

UNCLASSIFIED

DEFENCE RESEARCH ESTABLISHMENT SUFFIELD
RALSTON ALBERTA

SUFFIELD MEMORANDUM NO. 1104

AN INVESTIGATION OF THE SUITABILITY OF USING A SIEGLAFF-MCKELVEY HIGH SHEAR RATE MELT RHEOMETER FOR THE MEASUREMENT OF LOW VISCOSITY POLYMER SOLUTIONS (U)

by

J.B. Hacker

PREFACE

The following report was prepared by Mr. J.B. Hacker as part of the requirement for co-operative student education in the Faculty of Engineering, University of British Columbia. The work was performed under the direction of Dr. S.J. Armour at the Defence Research Establishment Suffield during May – August, 1983.

DEFENCE RESEARCH ESTABLISHMENT SUFFIELD
RALSTON ALBERTA

SUFFIELD MEMORANDUM NO. 1104

AN INVESTIGATION OF THE SUITABILITY OF USING A SIEGLAFF-MCKELVEY HIGH SHEAR RATE MELT RHEOMETER FOR THE MEASUREMENT OF LOW VISCOSITY POLYMER SOLUTIONS (U)

by

J.B. Hacker

ABSTRACT

An investigation was made into the adaptation of a Sieglaff-McKelvey high shear rate melt rheometer for use in measuring low viscosity fluids. Using calibrated Newtonian oils, viscosities as low as 1.5 poise were found to be measurable with better than 5% accuracy over a shear rate range from a nominal 1000 1/S to 100,000 1/S at temperatures as low as 5°C above ambient. However, difficulties were experienced in the measurement of low viscosity polymer solutions. With the stock capillaries 25.40 mm in length, a combination of wall slip and entrance/exit effects made calculating true viscosities impossible. It was concluded that capillaries with a diameter of 1.0 mm or greater and variable lengths of up to 50 mm would be required to eliminate slip and still obtain a pressure drop within the measurable range of the instrument. To facilitate accurate measurement of low pressure drops, a new piston design was proposed using low-friction, low leakage Teflon o-rings. This would also expand the lower limits of the instrument's viscosity and shear rate ranges.

TABLE OF CONTENTS

Page No.

PREFACE

ABSTRACT

TABLE OF CONTENTS

LIST OF APPENDICES

LIST OF FIGURES

INTRODUCTION 1

INSTRUMENT DESCRIPTION 2

THEORY 3

I General Concepts 3

II Capillary Flow Viscometry — Non-Newtonian Fluids 4

EXPERIMENTAL 6

CONCLUSIONS 8

RECOMMENDATIONS 9

REFERENCES 10

APPENDICES

FIGURES

LIST OF APPENDICES

APPENDIX A. Piston Dimensions

APPENDIX B. Capillary Dimensions

APPENDIX C. Viscosity of Standardized Newtonian Oils at 40.0°C

APPENDIX D. Shear Rate and Pressure Drop Data at 40.0°C

APPENDIX E. Bagley End Correction

APPENDIX F. Bagley End Correction

APPENDIX G. Bagley End Correction

APPENDIX H. Slip Co-Efficient (β)

APPENDIX I. Slip/No Slip Shear Rates

LIST OF FIGURES

FIGURE 1. Sieglaff-McKelvey High Shear Rate Rheometer

FIGURE 2. Cylinder Barrel, Piston and Capillaries

FIGURE 3. Log Viscosity vs Log Shear Rate Plot for a Typical Shear Thinning Polymer

FIGURE 4. Capillary Velocity Profiles With and Without Slip

FIGURE 5. Pressure Drop vs Shear Rate Plot for a Newtonian Oil

FIGURE 6. Viscosity vs Shear Rate Plots for Five Newtonian Oils

FIGURE 7. Pressure Drop vs Shear Rate Plots for Dowanol DPM/PMMA

FIGURE 8. Bagley Plot for Dowanol DPM/PMMA

FIGURE 9. Slip Co-Efficient vs Shear Rate Plot for Dowanol DPM/PMMA

FIGURE 10. Current and Proposed Capillary Designs

FIGURE 11. Current and Proposed Piston Tips

DEFENCE RESEARCH ESTABLISHMENT SUFFIELD
RALSTON ALBERTA

SUFFIELD MEMORANDUM NO. 1104

AN INVESTIGATION OF THE SUITABILITY OF USING A SIEGLAFF-MCKELVEY HIGH SHEAR RATE MELT RHEOMETER FOR THE MEASUREMENT OF LOW VISCOSITY POLYMER SOLUTIONS (U)

by

J.B. Hacker

INTRODUCTION

1. The Sieglaff-McKelvey Capillary Rheometer marketed by Imass Inc. is a commercial instrument intended for the measurement of the viscosity of polymer melts at high shear rates and at temperatures well above ambient. Because the interests of the Physical Chemistry Group at the Defence Research Establishment Suffield (DRES) lie in the behaviour of low-viscosity polymer fluids approximately two to three orders of magnitude thinner than melts and at temperatures much closer to ambient, an investigation was made into the suitability of using this rheometer to measure such fluids. It was hoped not only to determine the applicability of using this instrument for low-viscosity polymer solutions, but also to determine the limits of viscosity, shear rate, and temperature ranges of the instrument.

INSTRUMENT DESCRIPTION

2. The Sieglaff-McKelvey High Shear Rate Capillary Rheometer uses the principle of flow through a tube to measure fluid viscosities. It is a two piece instrument consisting of a rigid cast iron loading frame and a control and recording console (Figure 1).

3. The loading frame houses a pneumatically operated piston which fits into a replaceable stainless steel cylinder barrel. A number of piston diameters are available from 6.35 mm to 12.70 mm, the largest of which requires approximately 10 mL of fluid (Appendix A). Small diameter capillaries of 25.40 mm in length are screwed tightly into the bottom of the cylinder barrel. A selection of capillary diameters are available from 0.30 mm to 1.80 mm and are constructed out of pressed in precision bore tubing (Figure 2). The diameters are calibrated to 5 digit accuracy at the factory (Appendix B).

4. The control console is divided into three main sub-sections: (1) piston drive control; (2) temperature regulation; (3) the recording system.

5. The piston drive consists of a pneumatic valve to control the direction of piston travel and a pressure regulator and gauge to regulate the force exerted by the piston when in the constant stress mode. Alternatively, a needle valve on the loading frame may be used to control piston velocity in the constant rate mode.

6. The electronic temperature regulator contains potentiometers to pre-set the desired temperature and a digital display to indicate either pre-set or sample temperature. Temperature control is affected by changing the duty cycle of the resistance-type elements.

7. The recording system consists of a high speed Hewlett-Packard Model 7402A 2-pen oscillographic recorder for a permanent record of both piston velocity and piston load. Two piston load cells are available covering a range from 0 – 900 N and 0 – 9000 N, and are easily interchanged.

8. The two bench top units are interconnected by electrical cables and pressure hoses for the pneumatic drive. The instrument requires clean compressed air or nitrogen at 6 to 7 bar pressure for dependable operation.

THEORY

1. General Concepts

9. In rheology, the study of the flow and deformation of materials, the most broad characterization of fluids is whether they are Newtonian or Non-Newtonian.

10. Newtonian fluids are typified by low molecular mass liquids such as water, oils and most solvents. The shear viscosity of a Newtonian fluid is dependent on temperature only; the higher the temperature, the thinner, or less viscous, the fluid. This change in viscosity with temperature follows approximately Andrade's law which for Newtonian fluids is (Reference 1):

$$\eta = ae^{-b/T} \qquad [1]$$

Because of this sensitivity, viscosities are always quoted at a specific temperature. The viscosity of Newtonian fluids in steady shear is easily measured on a number of very accurate, simple, commercial instruments. As a result these fluids are often used as calibrating standards for more complex rheometers.

11. Non-Newtonian fluids, however, are somewhat more complicated. These fluids exhibit shear dependent viscosity and most are either shear thickening or shear thinning. That is, their viscosity at a constant temperature either increases or decreases as the shear rate is increased. Thus, to characterize the viscosity flow curve for a Non-Newtonian fluid, it is necessary to measure the viscosity over a wide range of shear rates at the desired temperature. Shear rates are measured in units of reciprocal seconds (1/S), and the ability to measure the range from 0 to 100,000 1/S is generally required to fully characterize a fluid. At the upper and lower extremes of the shear rate range, the viscosity of most Non-Newtonian fluids approaches limiting viscosities known respectively as the infinite shear viscosity and the zero shear viscosity (Figure 3). Since most fluids of interest to DRES are Non-Newtonian in behaviour, it was hoped that the Sieglaff-McKelvey Capillary Rheometer could be used to determine infinite shear viscosities by measuring viscosities in the upper shear rate range from approximately 1000 1/S to 100,000 1/S, a range unobtainable with other instruments in the laboratory.

II. Capillary Flow Viscometry — Non-Newtonian Fluids

12. To determine shear viscosity, it is necessary to evalute both the shear stress and the shear rate at some convenient point in the capillary, usually the wall. The classical formula for shear stress at the wall of a capillary is the so-called "Poiseuille Law" (Reference 2):

$$\tau_\omega = \frac{R_c \Delta P}{2L_c} \qquad [2]$$

where τ_ω = shear stress at the wall

ΔP = pressure drop due to viscous losses

R_c = capillary radius

L_c = capillary length

13. To be valid this equation requires steady laminar flow with straight flow streamlines and no change in velocity in the direction of flow. Because such idealistic assumptions are rarely met in working capillary rheometers, particularly with Non-Newtonian fluids, several corrections are typically employed.

14. The most important correction which takes into account both the entrance and exit flow losses and the elastic potential energy acquired by the fluid durir.g steady flow can be evaluated using a method first developed by Bagley (Reference 3). This method determines an equivalent extra length (L_e) of tube which would have to be added to the actual length if the total measured pressure drop were that for an entirely fully developed region.

15. Since from equation [2]

$$\Delta P = 2\,\tau_\omega \left(\frac{L_c}{R_c} + \frac{L_e}{R_c} \right) \qquad [3]$$

and noting shear stress (τ_ω) is a unique function of shear rate, the end correction (L_e/R_c) can be evaluated for Non-Newtonian fluids by plotting pressure drop versus L_c/R_c using data from a number of different capillaries at a constant shear rate and extrapolating back to the x-axis to obtain the equivalent extra length (L_e). It should be noted that this is usually done using a constant capillary radius (R_c) with variable

lengths (L_c) to obtain different values of L_c/R_c. However due to the design of the Sieglaff-McKelvey Rheometer, the lengths were not variable and different radii had to be used instead.

16. A second correction must often be made for the kinetic energy gain in the fluid as it is accelerated from rest to its exit velocity at the end of the capillary. However, due to the low flow rates employed by the Sieglaff-McKelvey, error due to this effect was below 0.05% and considered negligible.

17. The classical wall shear rate equation for Newtonian fluids having a fully developed parabolic velocity profile within the capillary is given by (Reference 2):

$$\Gamma = \frac{4Q}{\pi R_c^3} \qquad [4]$$

where Γ = Newtonian wall shear rate

Q = flow rate

R_c = capillary radius

and (Reference 4):

$$Q = \frac{V_p}{\pi R_p^2} \qquad [5]$$

where V_p = piston velocity

R_p = piston radius

18. For Non-Newtonian fluids, the velocity profile will not be a true parabola and a correction known as the Rabinowitsch equation must be applied as follows (Reference 2):

$$\dot{\gamma}_\omega = \left[\frac{3n' + 1}{4n'}\right]\Gamma \qquad [6]$$

where $\dot{\gamma}_\omega$ = wall shear rate

and

$$n' = \frac{d\ln\tau_\omega}{d\ln\Gamma} \qquad [7]$$

19. An additional problem with Non-Newtonian fluids is slip at the wall of the capillary. For true laminar flow within the capillary, the velocity profile must be a smooth curve with a maximum velocity at the centre and zero velocity at the wall. When slip occurs the velocity is no longer zero at the wall but some finite value (Figure 4). This effect may be accounted for by assuming an effective slip velocity superimposed upon the fluid in the tube and using a revised version of the Rabinowitsch equation employing a no-slip shear rate (Reference 2):

$$\Gamma_{no\ slip} = \Gamma_{measured} - \frac{4\beta\tau_\omega}{R_c} \qquad [8]$$

where β, the slip-coefficient, is the slope of the graph of $\Gamma/4\tau_\omega$ versus $1/R_c$ and a function of shear stress.

20. It should be noted that the slip correction may not be applied if the end correction is not negligible. As a general rule of thumb, slip can be avoided simply by using capillaries of sufficiently large diameter, typically greater than 1.0 mm.

21. From the values of shear stress and shear rate at the wall, the viscosity can be calculated using the equation (Reference 2):

$$\eta = \frac{\tau_\omega}{\dot{\gamma}_\omega} \qquad [9]$$

where η = viscosity

22. Thus by calculating the viscosity over a range of shear rates, a plot of viscosity versus shear rate of the test fluid may be constructed and any limiting viscosity easily determined.

EXPERIMENTAL

23. As an initial attempt to gauge the accuracy of the rheometer, and to determine the lower limit of its viscosity range, a series of tests were run using Newtonian oils of known viscosity at 40.0°C. Viscosities ranged from 200 poise to 1.5 poise and capillary diameters from 0.30 to 0.60 mm were used. From the data recorded on the strip chart, plots of pressure drop (ΔP) versus shear rate (Γ) were made and the best straight line fitted using the least squares method. A typical plot is shown in Figure 5. From the

equation of this line and the capillary dimensions viscosities were calculated and compared with the certified National Bureau of Standards (NBS) viscosity at the same temperature (Appendix C and Figure 6).

24. From these runs it was determined that viscosities as low as 1 poise were measurable, though less accurately, as the pressure drops became masked by inconsistencies such as piston friction and leakage. In all cases accuracy was better than 5%.

25. It was also determined that Newtonian shear rates (Γ) from a nominal 1000 1/S to 100,000 1/S were obtainable, the lower limit being an inverse function of the test sample viscosity and ranging from 200 1/S for the 200 poise oil to 2000 1/S for the 1.5 poise oil.

26. As viscosity for most fluids is very sensitive to temperature, extensive testing and calibration of the temperature regulation was done. A calibrated digital thermocouple (Cole-Parmer model 8502-25) accurate to $\pm$ 0.05°C was used to measure temperatures within the cylinder barrel. Results indicated a temperature variation of $\pm$ 0.3°C along the length of the cylinder barrel from the value as read on the digital display of the control console.

27. A thermocouple was also inserted into the capillary itself, and variations of less than $\pm$ 0.1°C were noted. Thus, temperature regulation, once calibrated, was judged to be adequate for the accuracy expected from the instrument ($\pm$ 5%).

28. With the basic limits of the rheometer now established, a representative Non-Newtonian fluid was run. The chosen fluid was a well documented 41 g/L polymer solution of Dowanol DPM (dipropylene glycol methyl ether) thickened with a polymethyl methacrylate (PMMA) having a weight average molecular weight of 2×10^6.

29. As before, pressure drop versus shear rate plots were made at 40.0°C, this time using the three smallest diameter capillaries. The nominal diameters of these capillaries ranged from 0.30 mm to 0.50 mm with lengths of 25.40 mm. The plots were found to be linear with positive y-intercepts over the measured shear rate range from 2000 1/S to 80,000 1/S (Appendix D and Figure 7).

30. However, when the Bagley end correction was attempted, the results indicated both a positive or negative end correction length depending on shear rate, an anomalous result (Appendices E, F, G and Figure 8). This suggested the presence of slip and subsequently the slip correction was carried out. However, it too gave anomalous results in the form of a negative slip velocity for the lower shear rates (Appendices H, I and Figure 9).

31. The problem appeared to be both slip and end effect related and thus neither correction by itself was adequate. Thus, the only recourse was to alter the physical parameters, L_c and R_c, of the capillaries.

32. In an attempt to eliminate the slip, capillaries of larger diameter (D = 0.50 mm) were tried but due to their short length (25.40 mm) it became impossible to separate the very low pressure drops from other noise during a run. The manufacturer, Tinius Olsen Testing Machine Company, was then contacted but was unable to supply longer capillaries from stock. As a result, the experimentation was terminated until longer capillaries could be obtained or built. The new capillaries would have lengths of up to 50 mm and diameters greater than 0.50 mm. As the present furnace was designed primarily for capillaries of 25.40 mm in length, lengths of greater than 50 mm would present either problems in temperature control without major modifications to the present set up or a dramatic decrease in piston travel and hence test fluid capacity.

CONCLUSIONS

33. It was concluded that the Sieglaff-McKelvey Capillary Rheometer can accurately measure viscosities of Newtonian fluids as low as 1.5 poise and at shear rates from a nominal 1000 1/S to 100,000 1/S, and at temperatures as low as 5°C above ambient. The accuracy of these measurements was found to be better than 5% in every case.

34. It was also concluded that while it is possible to adapt the Sieglaff-McKelvey Capillary Rheometer to measure low viscosity polymer solutions at near ambient temperatures, such a conversion would require capillaries of greater length than those currently stocked by the manufacturer.

35. It was found that an increase in the signal to noise ratio of the piston load channel would allow the use of larger diameter capillaries by allowing the accurate measurement of very low pressure drops. Such an improvement would be especially

significant for Non-Newtonian fluids where large diameter capillaries are necessary to prevent slip from occurring. As a bonus, such an improvement would also expand the lower limits of the instrument's viscosity and shear rate ranges.

RECOMMENDATIONS

36. A number of recommendations are suggested to make the Sieglaff-McKelvey Capillary Rheometer more suited to the requirements of the DRES Physical Chemistry laboratory.

37. These include a modification to accept variable length capillaries such as that shown in Figure 10. A modified piston tip employing low friction Teflon o-rings to decrease both piston friction and leakage thereby improving the sensitivity of the piston load channel (Figure 11). A recirculating water/ethylene glycol environmental chamber might be designed to allow sub-ambient temperatures to be obtained, an impossibility with the present set-up. Finally, an electronic servo system to allow preprogrammed computer controlled runs could be built. A dedicated computer could also be used to handle data analysis directly off the instrument avoiding the present system of strip chart recordings and human interpretation, a lengthy and potentially error prone process.

38. With some or all of these modifications, the Sieglaff-McKelvey Capillary Rheometer would fulfill the initial requirements of the DRES Physical Chemistry laboratory.

REFERENCES

1. Eirich, F.R., **"Rheology, Theory and Applications"**, Academic Press Limited, 1960.

2. Darby, Ronald, **"Viscoelastic Fluids"**, Marcel Dekker Inc., 1976.

3. Bagley, E.B., **"End Corrections in the Capillary Flow of Polyethylene"**, J. Appl. Phys. 28, 624 (1957).

4. **"Sieglaff-McKelvey Rheometer Instruction Manual 80-6"**, Tinius-Olsen Testing Machine Company, Inc.

5. Walters, K., **"Rheometry"**, Chapman and Hall Ltd., 1975.

6. Whorlow, R.W., **"Rheological Techniques"**, Ellis Horwood, 1980.

7. Philipoff, W. and Gaskins, F., **"The Capillary Experiment in Rheology"**, Transactions of the Society of Rheology II, pp 263-284, 1958.

8. Boger, D.V., Gupta, R. and Tanner, R.I., **"The End Correction for Power-Law Fluids in the Capillary Rheometer"**, Journal of Non-Newtonian Fluid Mechanics, 4 (1978), pp 239 – 248.

APPENDIX A

Piston Dimensions

DESIGNATION	RADIUS (R_p) (mm)	AREA (A_p) (mm^2)
#1	3.18	31.7
#2	3.97	49.5
#3	6.35	126.7

APPENDIX B

Capillary Dimensions

DESIGNATION	RADIUS (R_c) (mm)	LENGTH (L_c) (mm)
A	0.15469	25.40
B	0.20633	25.40
C	0.25432	25.40
D	0.31002	25.40
E	0.38788	25.40
F	0.49018	25.40
G	0.62131	25.40
H	0.82201	25.40
J	0.82755	25.40
K	0.88960	25.40

APPENDIX C

Viscosity of Standardized Newtonian Oils at 40.0°C

η (NBS) (poise)	R_c (mm)	L_c (mm)	η (measured) (poise)	% error
200.3	0.15469	25.40	206.5	3.11
200.3	0.20633	25.40	199.8	– 0.27
67.44	0.15469	25.40	67.88	0.65
67.44	0.20633	25.40	68.20	1.13
67.44	0.25432	25.40	69.65	3.28
67.44	0.31002	25.40	68.57	1.68
13.89	0.15469	25.40	13.63	– 1.91
13.89	0.20633	25.40	13.70	– 1.73
13.89	0.25432	25.40	14.50	4.15
13.89	0.31002	25.40	14.03	1.03
4.203	0.15469	25.40	4.078	– 2.96
4.203	0.20633	25.40	4.063	– 3.32
4.203	0.25432	25.40	4.308	2.51
4.203	0.31002	25.40	4.320	2.89
1.494	0.15469	25.40	1.425	– 4.49
1.494	0.20633	25.40	1.439	– 3.69
1.494	0.25432	25.40	1.568	4.97

APPENDIX D

Shear Rate and Pressure Drop Data at 40.0°C

Sample: 40.89 g/L Dowanol DPM/PMMA

Capillary A: R_c = 0.15469 mm L_c = 25.40 mm

SHEAR RATE (Γ) (1/S)	PRESSURE DROP (ΔP) (dyne/cm²)	SHEAR RATE (Γ) (1/S)	PRESSURE DROP (ΔP) (dyne/cm²)
1946	1.381×10^6	20 068	5.723×10^6
3000	1.599×10^6	29 899	7.993×10^6
3943	1.887×10^6	41 047	1.058×10^7
5078	2.171×10^6	59 797	1.492×10^7
10014	3.442×10^6	79 257	1.875×10^7
15000	4.697×10^6		

Capillary B: R_c = 0.20633 mm L_c = 25.40 mm

SHEAR RATE (Γ) (1/S)	PRESSURE DROP (ΔP) (dyne/cm²)	SHEAR RATE (Γ) (1/S)	PRESSURE DROP (ΔP) (dyne/cm²)
1943	9.868×10^5	10 122	2.518×10^6
2998	1.172×10^6	15 290	3.552×10^6
3989	1.362×10^6	19 998	4.737×10^6
5108	1.626×10^6	29 982	6.473×10^6
6065	1.753×10^6	39 720	8.427×10^6
7859	2.289×10^6	60 648	1.303×10^7

Capillary C: R_c = 0.25432 mm L_c = 25.40 mm

SHEAR RATE (Γ) (1/S)	PRESSURE DROP (ΔP) (dyne/cm²)	SHEAR RATE (Γ) (1/S)	PRESSURE DROP (ΔP) (dyne/cm²)
1966	6.828×10^5	9 648	2.052×10^6
2965	8.762×10^5	15 050	2.999×10^6
4060	1.176×10^6	20 300	3.963×10^6
4995	1.263×10^6	24 997	5.032×10^6
5976	1.366×10^6	29 290	5.624×10^6
8028	1.760×10^6		

APPENDIX E

Bagley End Correction

Sample: 40.89 g/L Dowanol DPM/PMMA (40.0°C)

Capillary A: R_c = 0.15469 mm L_c = 25.40 mm

SHEAR RATE (Γ) (1/S)	$-L_e/R_c$	L_e (mm)	$\frac{L_e}{L_c} \times 100\%$
2000	49.6	− 7.67	− 30.2
3000	39.0	− 6.03	− 23.8
4000	29.4	− 4.55	− 17.9
5000	20.6	− 3.18	− 12.5
6000	12.6	− 1.95	− 7.67
8000	− 1.60	0.24	0.97
10 000	− 13.6	2.10	8.28
20 000	− 54.8	8.48	33.4
30 000	− 78.6	12.2	47.9
40 000	− 94.1	14.6	57.3
50 000	− 105.0	16.2	63.9
60 000	− 113.1	17.5	68.9
70 000	− 119.4	18.5	72.7
80 000	− 124.3	19.2	75.7

APPENDIX F

Bagley End Correction

Sample: 40.89 g/L Dowanol DPM/PMMA (40.0°C)

Capillary B: R_c = 0.20633 mm L_c = 25.40 mm

SHEAR RATE (Γ) (1/S)	$-L_e/R_c$	L_e (mm)	$\frac{L_e}{L_c} \times 100\%$
2000	49.6	– 10.2	– 40.3
3000	39.0	– 8.05	– 31.7
4000	29.4	– 6.07	– 23.9
5000	20.6	– 4.25	– 16.7
6000	12.6	– 2.60	– 10.2
8000	– 1.60	– 0.33	1.3
10 000	– 13.6	2.81	11.1
20 000	– 54.8	11.3	44.5
30 000	– 78.6	16.2	63.9
40 000	– 94.1	19.4	76.4
50 000	– 105.0	21.7	85.3
60 000	– 113.1	23.3	91.9
70 000	– 119.4	24.6	96.9
80 000	– 124.3	25.7	100.9

APPENDIX G

Bagley End Correction

Sample: 40.89 g/L Dowanol DPM/K125 EA (40.0°C)

Capillary C: R_c = 0.25432 mm L_c = 25.40 mm

SHEAR RATE (Γ) (1/S)	$-L_e/R_c$	L_e (mm)	$\frac{L_e}{L_c} \times 100\%$
2000	49.6	– 12.6	– 49.7
3000	39.0	– 9.92	– 39.1
4000	29.4	– 7.48	– 29.4
5000	20.6	– 5.24	– 20.6
6000	12.6	– 3.20	– 12.6
8000	– 1.60	0.41	1.6
10 000	– 13.6	3.46	13.6
20 000	– 54.8	13.9	54.9
30 000	– 78.6	20.0	78.7
40 000	– 94.1	23.9	94.2
50 000	– 105.0	26.7	105.1
60 000	– 113.1	28.8	113.2
70 000	– 119.4	30.4	119.6
80 000	– 124.3	31.6	124.5

APPENDIX H

Slip Co-Efficient (β)

Sample: 40.89 g/L Dowanol DPM/PMMA (40.0°C)

SHEAR STRESS (τ_ω) (dynes/cm^2)	β $\left(\frac{cm^3}{dyne \cdot s}\right)$	SHEAR STRESS (τ_ω) (dynes/cm^2)	β $\left(\frac{cm^3}{dyne \cdot s}\right)$
4 000	– 0.00403	30 000	0.00246
5 000	– 0.00253	40 000	0.00271
8 000	– 0.00029	50 000	0.00286
10 000	0.00046	60 000	0.00296
15 000	0.00146	70 000	0.00303
20 000	0.00196	80 000	0.00309

APPENDIX I

Slip/No Slip Shear Rates

Sample: 40.89 g/L Dowanol DPM/PMMA (40.0°C)

NO SLIP SHEAR RATE (Γ_{ns}) (1/S)	(Γ_s) CORRESPONDING UNCORRECTED SHEAR RATE (1/S)		
	CAPILLARY A	CAPILLARY B	CAPILLARY C
3000	84.4	347	672
4000	1700	1900	2170
5000	3320	3450	3660
6000	4940	5010	5160
8000	8180	7890	8150
10000	11420	11220	11140
20000	27600	26740	26110
30000	43800	42270	41070
40000	76180	73320	71000
60000	92370	88860	85960
70000	108600	104400	100900
80000	124800	119900	115900

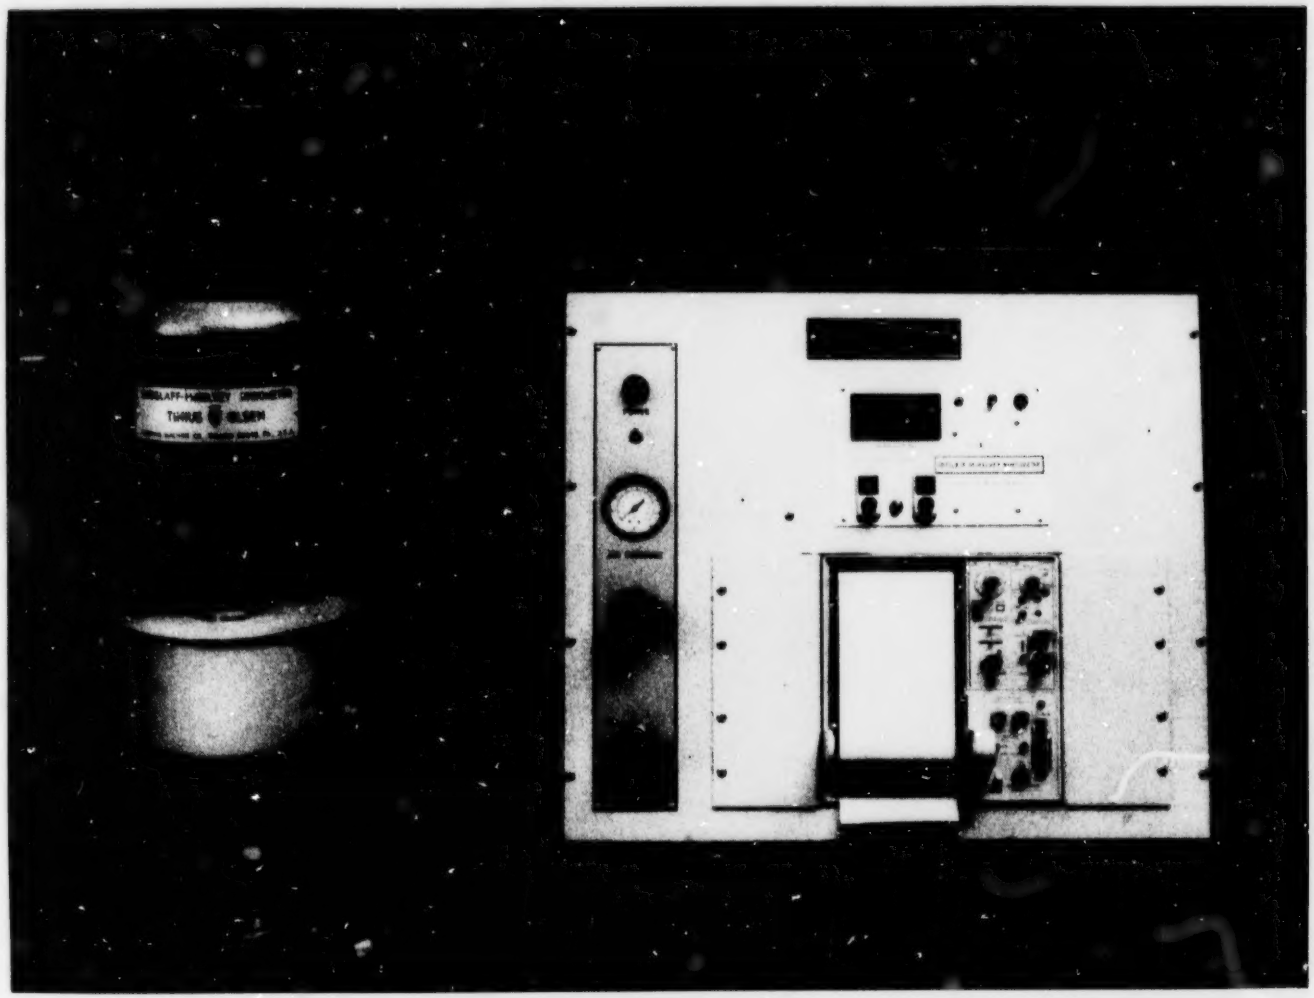

Figure 1

SIEGLAFF-McKELVEY HIGH SHEAR RATE RHEOMETER SHOWING LOADING FRAME (LEFT) AND CONTROL AND RECORDING CONSOLE (RIGHT)

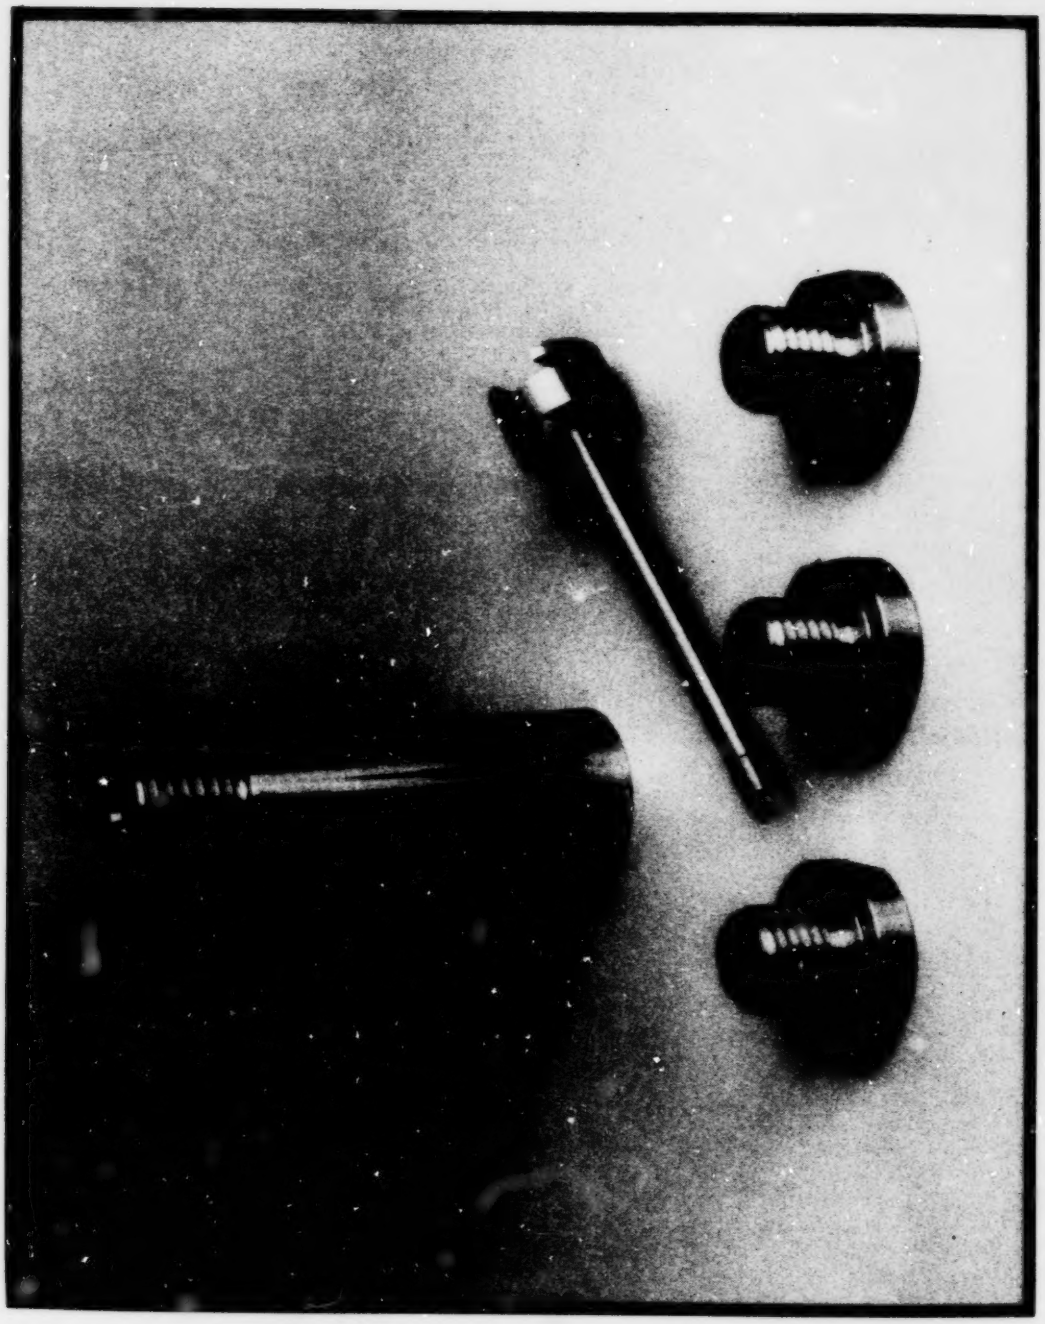

Figure 2

CYLINDER BARREL, PISTON AND CAPILLARIES FOR SIEGLAFF-McKELVEY RHEOMETER

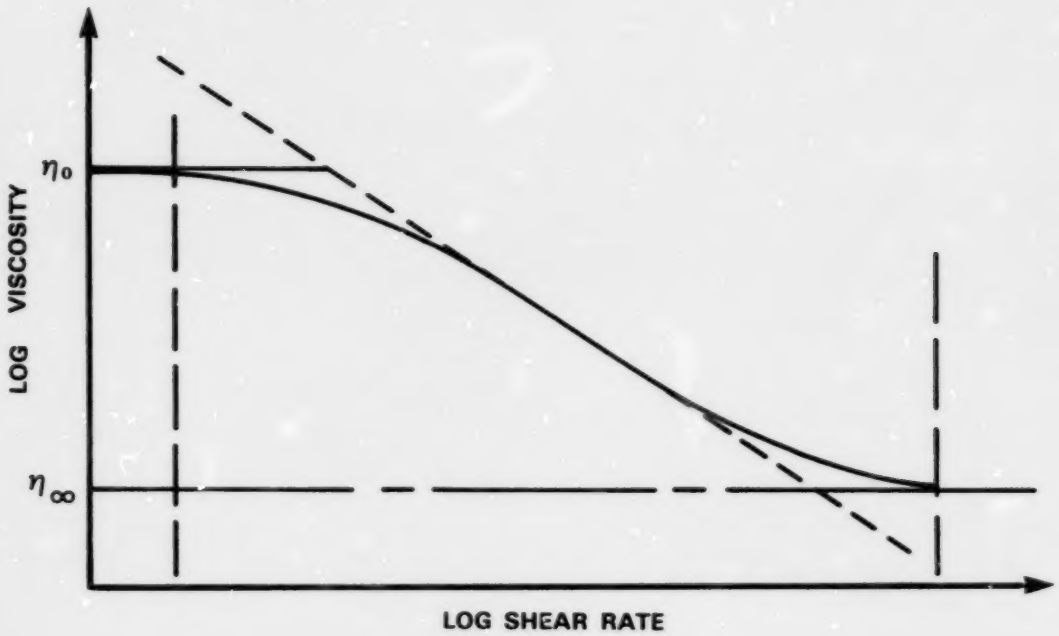

Figure 3

A PLOT OF LOG VISCOSITY VS LOG SHEAR RATE FOR A TYPICAL SHEAR THINNING POLYMER ILLUSTRATING ZERO SHEAR (η_0) AND INFINITE SHEAR (η_∞) VISCOSITIES

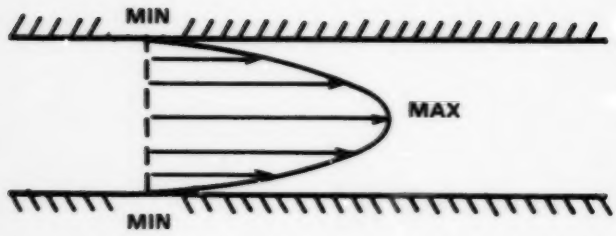

VELOCITY PROFILE WITHOUT SLIP

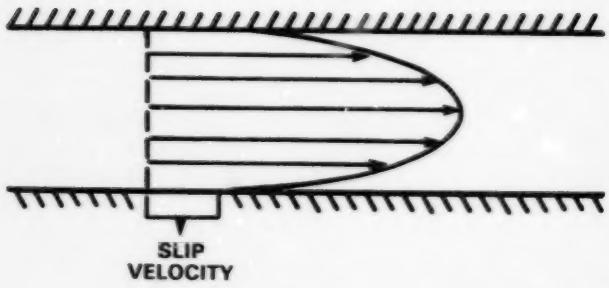

VELOCITY PROFILE WITH SLIP

Figure 4

CAPILLARY VELOCITY PROFILES WITH AND WITHOUT SLIP

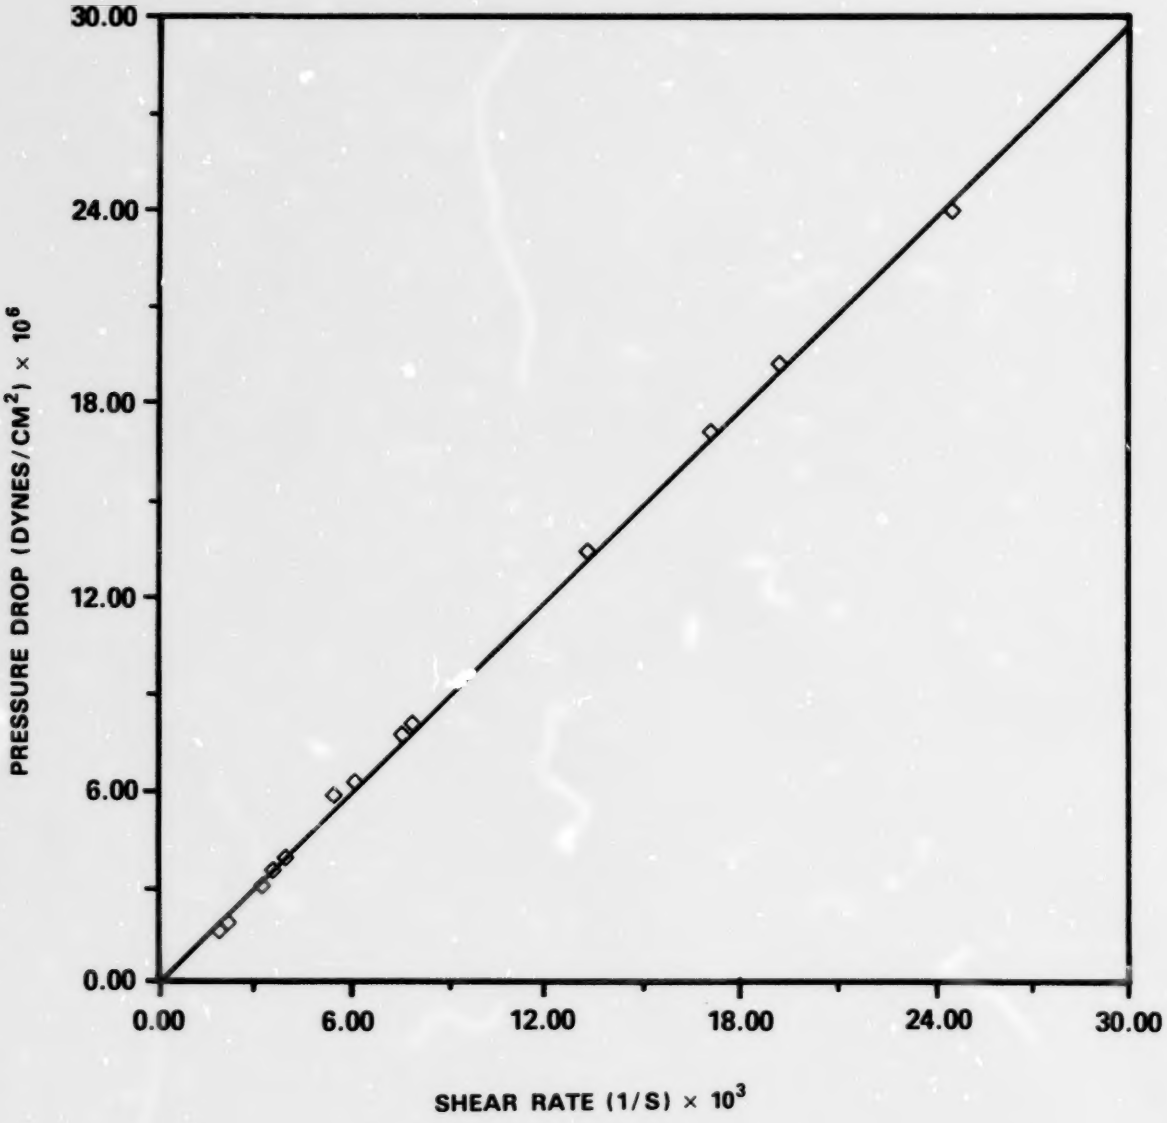

Figure 5

A TYPICAL PRESSURE DROP VS SHEAR RATE PLOT FOR A NEWTONIAN OIL. (CAPILLARY B; CANNON INSTRUMENT VISCOSITY STANDARD S 600, 4.203 POISE AT 40.0°C)

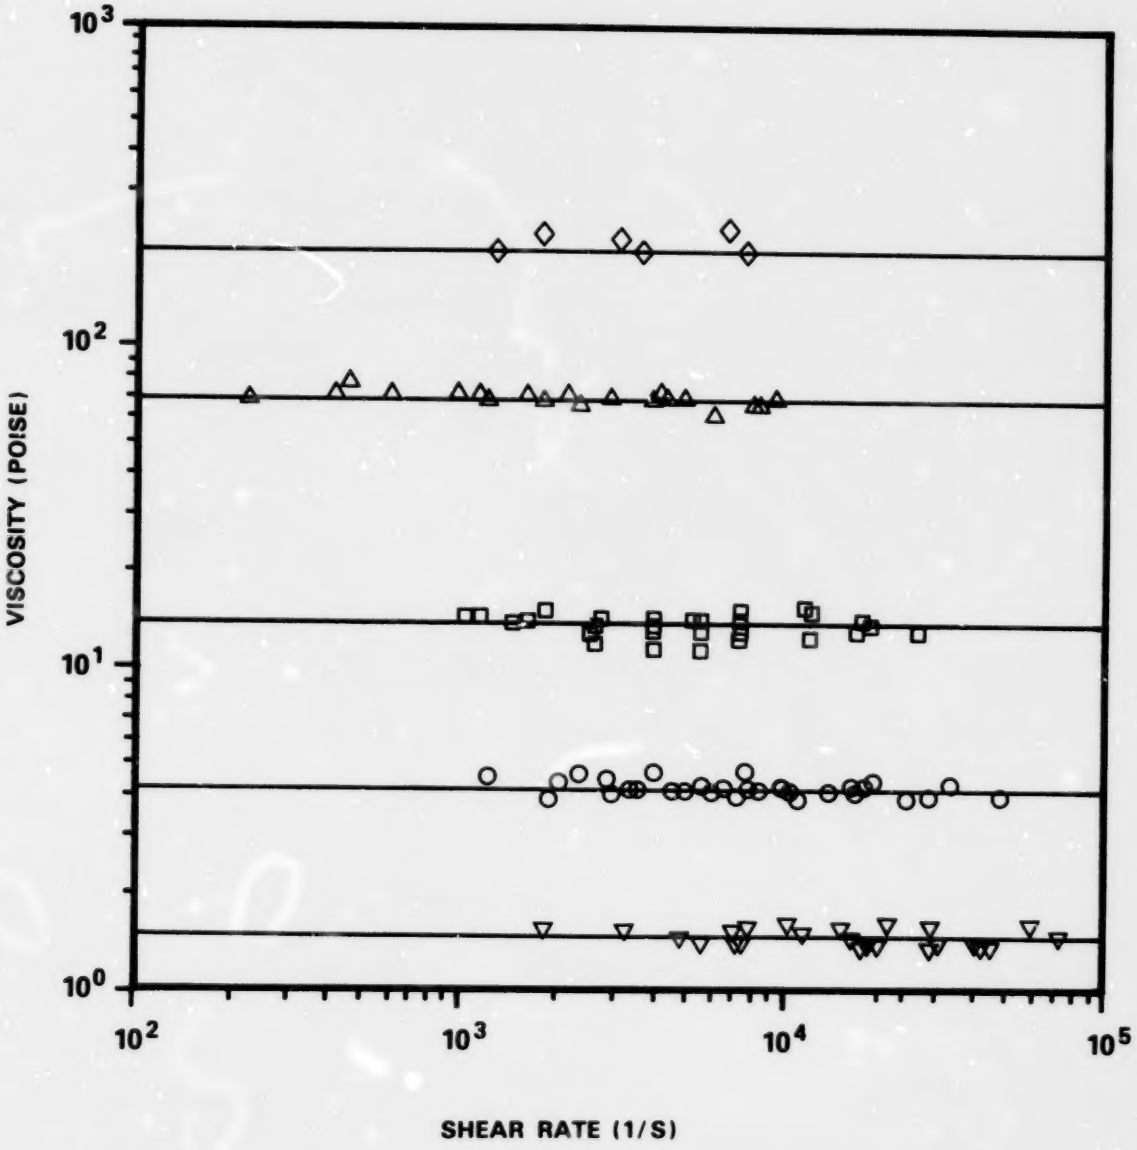

Figure 6

VISCOSITY VS SHEAR RATE PLOTS FOR FIVE NEWTONIAN OILS. LINES REPRESENT NBS VISCOSITY WHILE POINTS REPRESENT ACTUAL MEASURED VISCOSITIES USING SIEGLAFF-McKELVEY RHEOMETER (SEE APPENDIX C FOR AVERAGE VALUES)

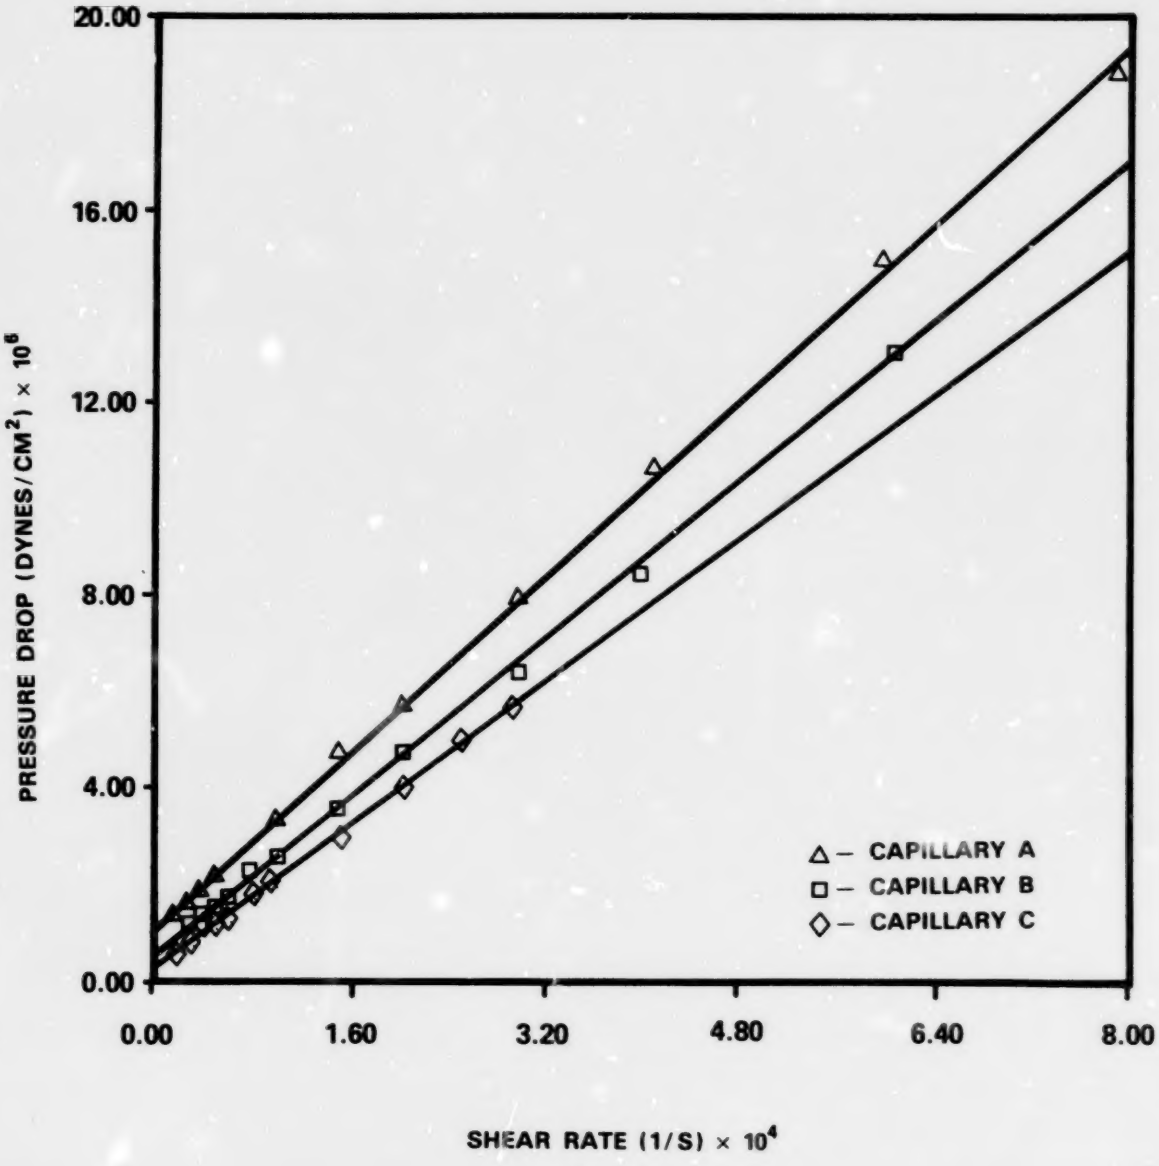

Figure 7

PRESSURE DROP VS NEWTONIAN SHEAR RATE PLOTS FOR 40.89 g/L DOWANOL DPM/PMMA AT 40.0°C

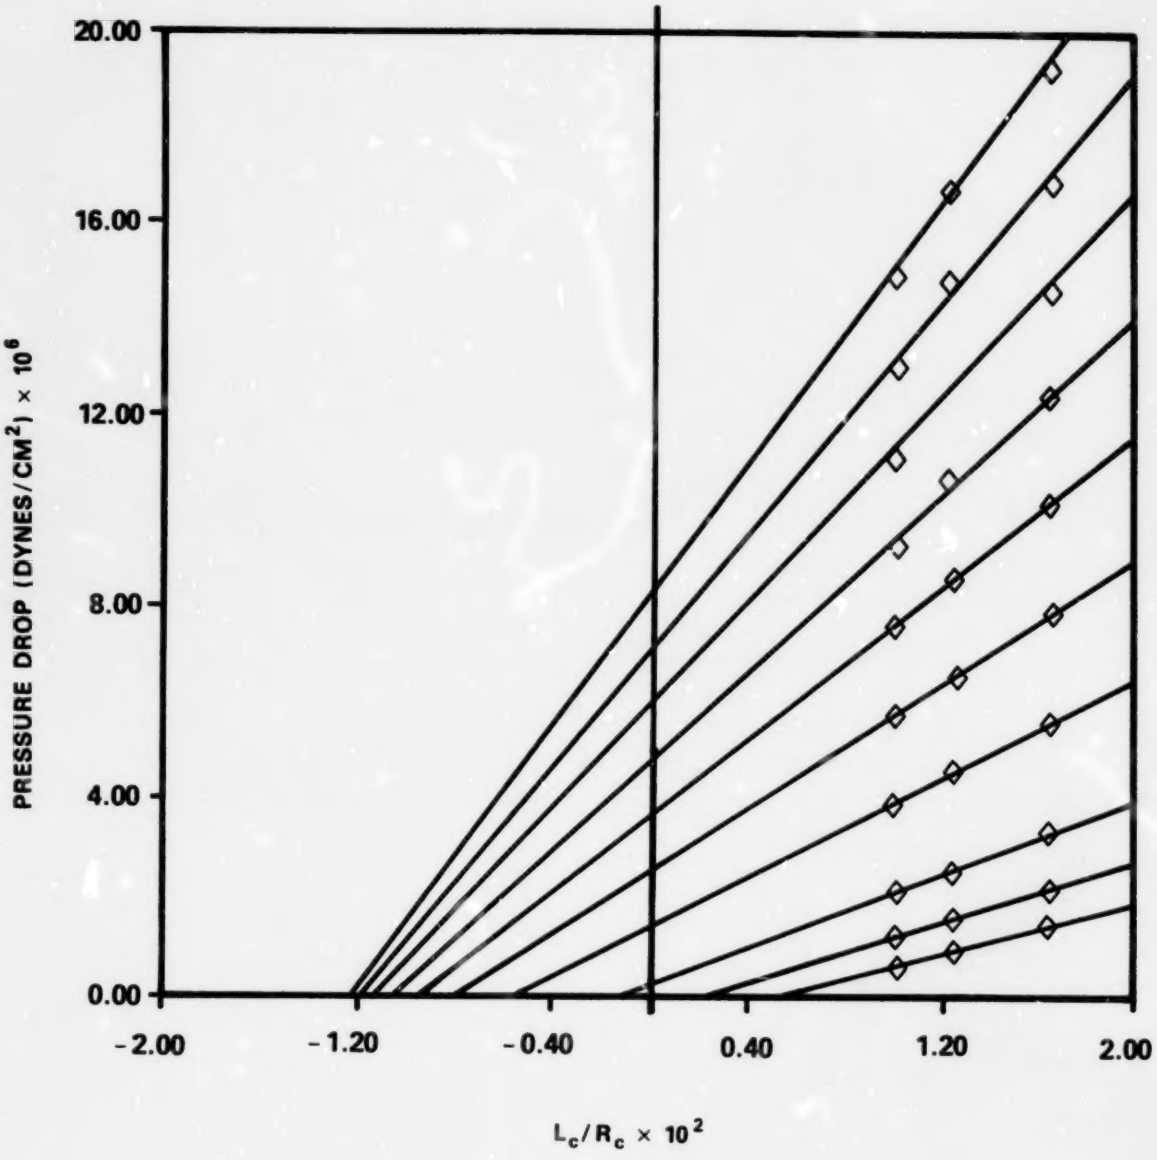

Figure 8

BAGLEY PLOT: PRESSURE DROP VS L_c/R_c FOR 40.89 g/L DOWANOL DPM/PMMA (40.0°C) AT TEN DIFFERENT SHEAR RATES. BY CALCULATING THE X-INTERCEPT THE VALUE OF L_e/R_c CAN BE DETERMINED.

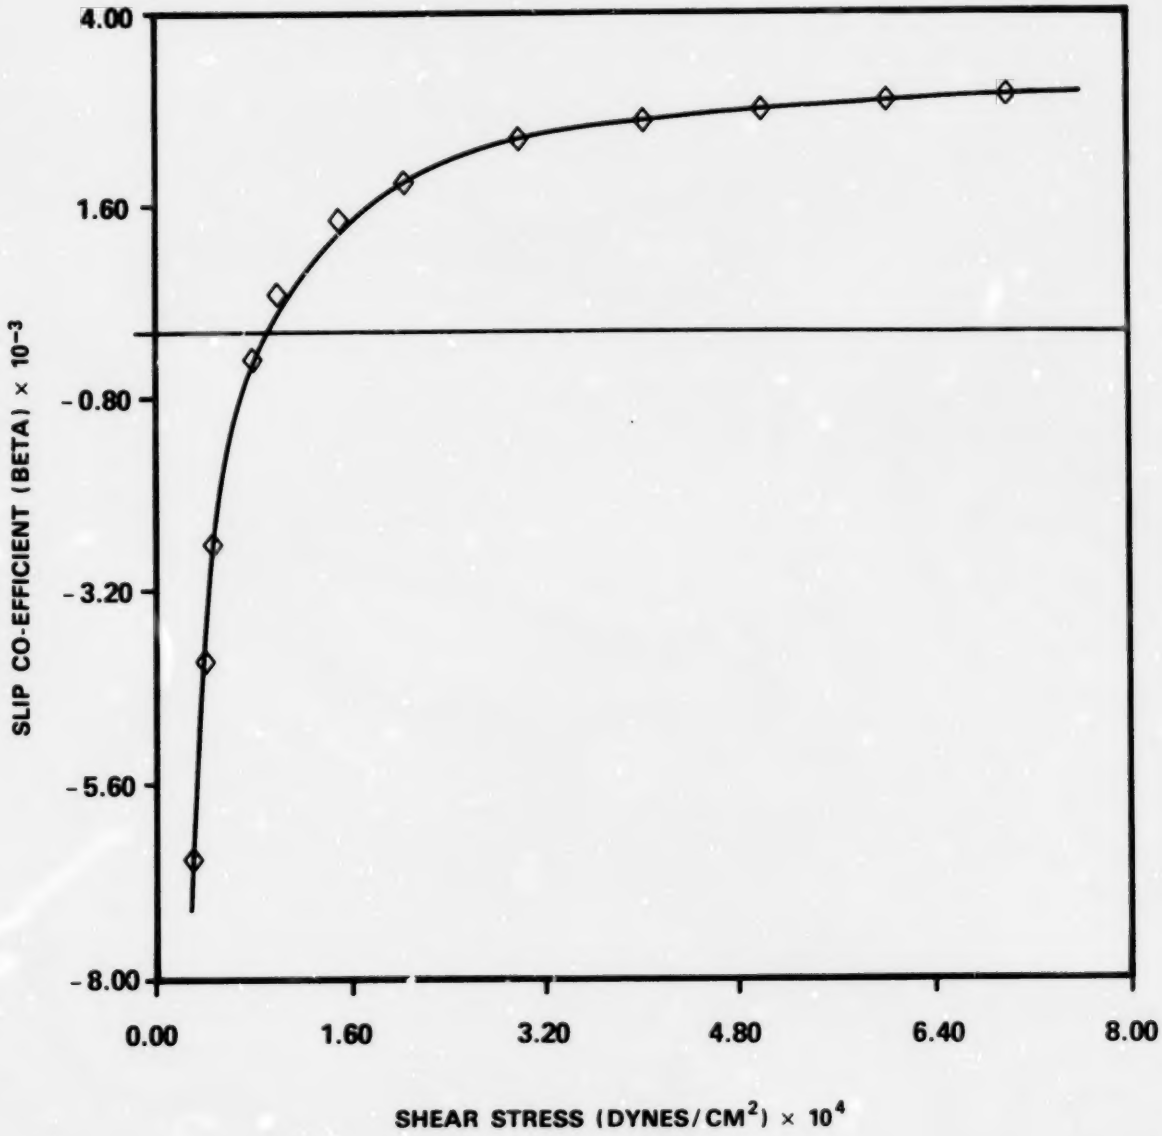

Figure 9

SLIP CO-EFFICIENT (BETA) AS A FUNCTION OF SHEAR STRESS FOR 40.89 g/L DOWANOL DPM/PMMA AT 40.0°C

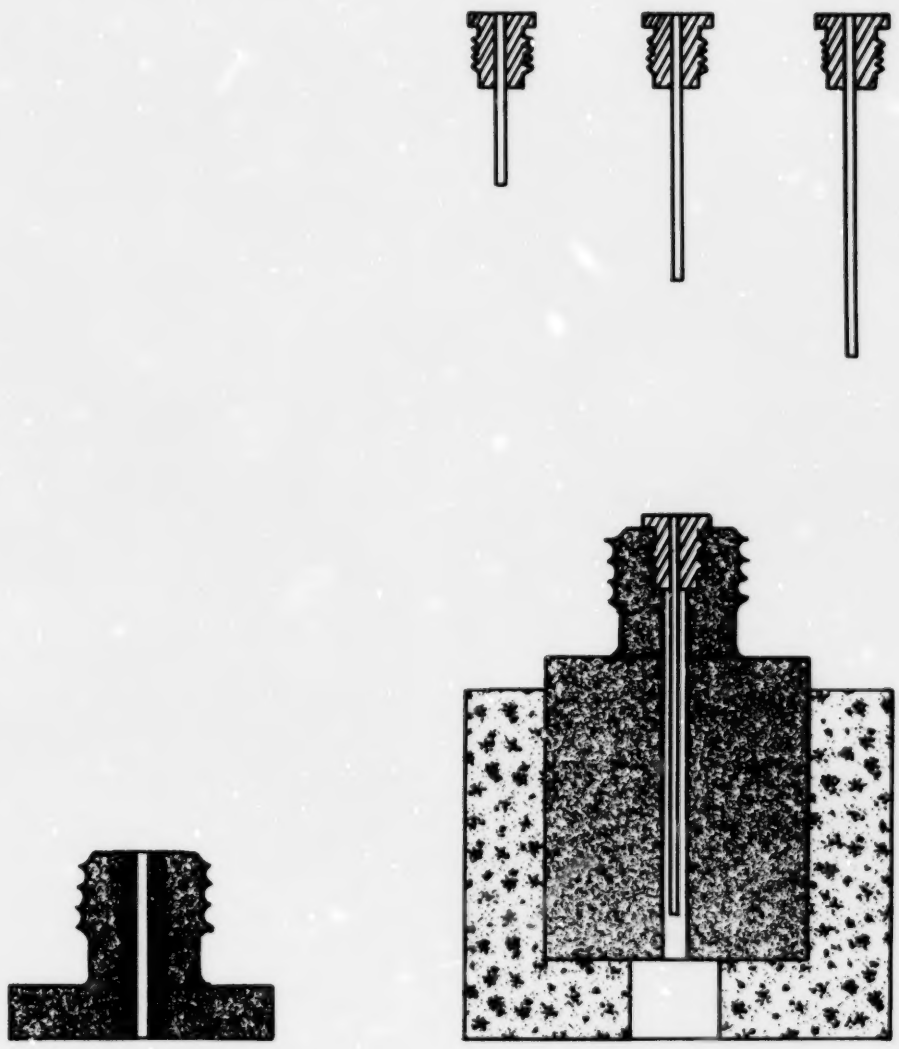

Figure 10

CURRENT CAPILLARY DESIGN (LEFT) AND VARIABLE LENGTH CAPILLARIES AND INSULATED HOLDER (RICHT)

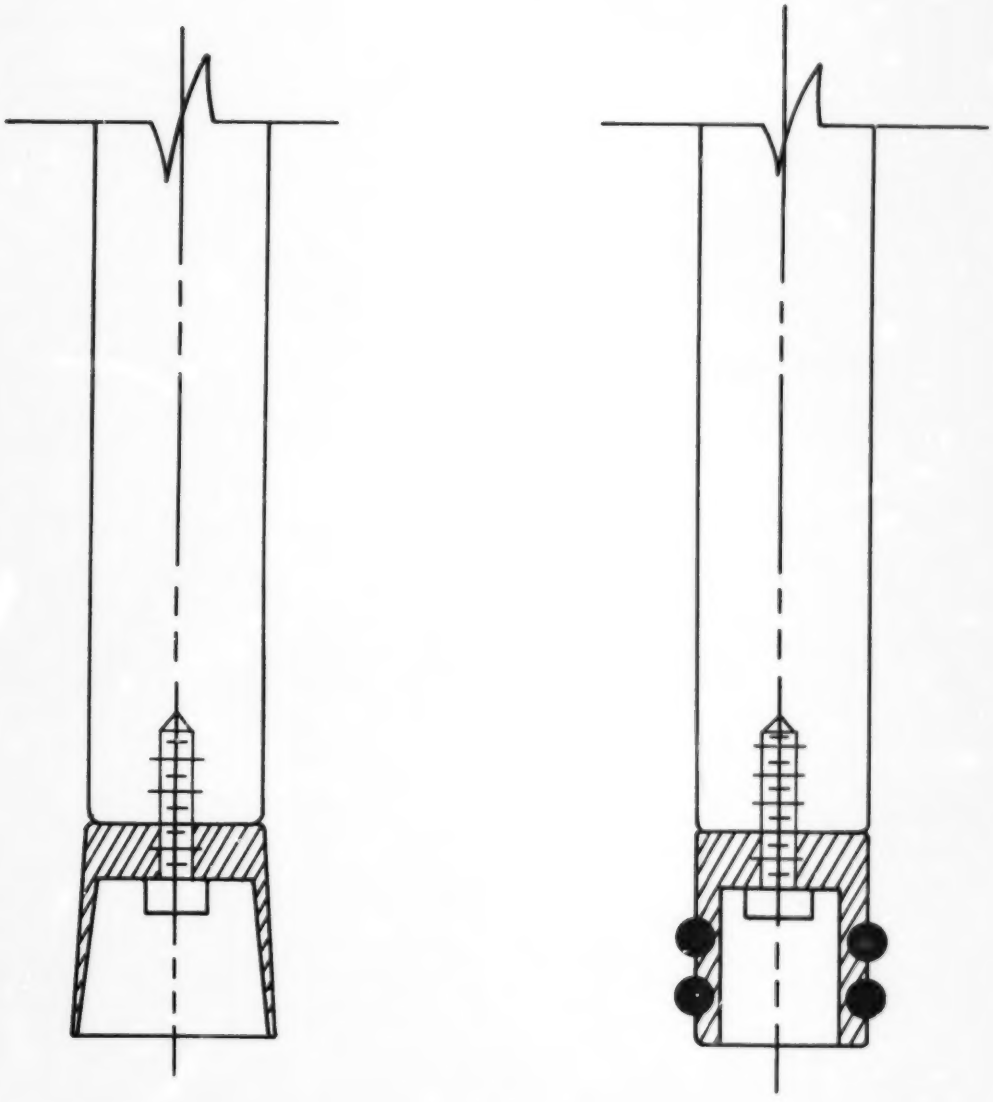

STANDARD BERYLLIUM-COPPER PISTON TIP

MODIFIED LOW FRICTION O-RING PISTON TIP

Figure 11

PISTON TIPS: STANDARD (LEFT) AND PROPOSED O-RING TYPE (RIGHT)

UNCLASSIFIED
This Sheet Security Classification

DOCUMENT CONTROL DATA - R & D
(Security classification of title, body of abstract and indexing annotation must be entered when the overall document is classified)

1 ORIGINATING ACTIVITY
Defence Research Establishment Suffield

2a. DOCUMENT SECURITY CLASSIFICATION
UNCLASSIFIED

2b. GROUP

3 DOCUMENT TITLE
AN INVESTIGATION OF THE SUITABILITY OF USING A SIEGLAFF-MCKELVEY HIGH SHEAR RATE MELT RHEOMETER FOR THE MEASUREMENT OF LOW VISCOSITY POLYMER SOLUTIONS

4 DESCRIPTIVE NOTES (Type of report and inclusive dates)
Suffield Memorandum

5 AUTHOR(S) (Last name, first name, middle initial)
Hacker, Jonathon B.

6 DOCUMENT DATE
August 1984

7a. TOTAL NO. OF PAGES

7b. NO. OF REFS
8

8a. PROJECT OR GRANT NO.
13E10

9a. ORIGINATOR'S DOCUMENT NUMBER(S)
SM 1104

8b CONTRACT NO.

9b. OTHER DOCUMENT NO.(S) (Any other numbers that may be assigned this document)

10. DISTRIBUTION STATEMENT
Unlimited

11. SUPPLEMENTARY NOTES

12. SPONSORING ACTIVITY

13. ABSTRACT

An investigation was made into the adaptation of a Sieglaff-McKelvey high shear rate melt rheometer for use in measuring low viscosity fluids. Using calibrated Newtonian oils, viscosities as low as 1.5 poise were found to be measurable with better than 5% accuracy over a shear rate range from a nominal 1000 1/S to 100,000 1/S at temperatures as low as 5°C above ambient. However, difficulties were experienced in the measurement of low viscosity polymer solutions. With the stock capillaries 25.40 mm in length, a combination of wall slip and entrance/exit effects made calculating true viscosities impossible. It was concluded that capillaries with a diameter of 1.0 mm or greater and variable lengths of up to 50 mm would be required to eliminate slip and still obtain a pressure drop within the measurable range of the instrument. To facilitate accurate measurement of low pressure drops, a new piston design was proposed using low-friction, low leakage teflon o-rings. This would also expand the lower limits of the instrument's viscosity and shear rate ranges. (U)

DSIR
78-679

KEY WORDS

high shear rate viscometer
Sieglaff-McKelvey viscometer
Newtonian liquids
polymer solutions
rheology

INSTRUCTIONS

1. ORIGINATING ACTIVITY. Enter the name and address of the organization issuing the document.

2a. DOCUMENT SECURITY CLASSIFICATION. Enter the overall security classification of the document including special warning terms whenever applicable.

2b. GROUP. Enter security reclassification group number. The three groups are defined in Appendix 'M' of the DRB Security Regulations.

3. DOCUMENT TITLE. Enter the complete document title in all capital letters. Titles in all cases should be unclassified. If a sufficiently descriptive title cannot be selected without classification, show title classification with the usual one-capital-letter abbreviation in parentheses immediately following the title.

4. DESCRIPTIVE NOTES. Enter the category of document, e.g. technical report, technical note or technical letter. If appropriate, enter the type of document, e.g. interim, progress, summary, annual or final. Give the inclusive dates when a specific reporting period is covered.

5. AUTHOR(S). Enter the name(s) of author(s) as shown on or in the document. Enter last name, first name, middle initial. If military, show rank. The name of the principal author is an absolute minimum requirement.

6. DOCUMENT DATE. Enter the date (month, year) of Establishment approval for publication of the document.

7a. TOTAL NUMBER OF PAGES. The total page count should follow normal pagination procedures, i.e., enter the number of pages containing information.

7b. NUMBER OF REFERENCES. Enter the total number of references cited in the document.

8a. PROJECT OR GRANT NUMBER. If appropriate, enter the applicable research and development project or grant number under which the document was written.

8b. CONTRACT NUMBER. If appropriate, enter the applicable number under which the document was written.

9a. ORIGINATOR'S DOCUMENT NUMBER(S). Enter the official document number by which the document will be identified and controlled by the originating activity. This number must be unique to this document.

9b. OTHER DOCUMENT NUMBER(S). If the document has been assigned any other document numbers (either by the originator or by the sponsor), also enter this number(s).

10. DISTRIBUTION STATEMENT. Enter any limitations on further dissemination of the document, other than those imposed by security classification, using standard statements such as:

(1) "Qualified requesters may obtain copies of this document from their defence documentation center."

(2) "Announcement and dissemination of this document is not authorized without prior approval from originating activity."

11. SUPPLEMENTARY NOTES. Use for additional explanatory notes.

12. SPONSORING ACTIVITY. Enter the name of the departmental project office or laboratory sponsoring the research and development. Include address.

13. ABSTRACT. Enter an abstract giving a brief and factual summary of the document, even though it may also appear elsewhere in the body of the document itself. It is highly desirable that the abstract of classified documents be unclassified. Each paragraph of the abstract shall end with an indication of the security classification of the information in the paragraph (unless the document itself is unclassified) represented as (TS), (S), (C), (R), or (U).

The length of the abstract should be limited to 20 single-spaced standard typewritten lines; 7½ inches long.

14. KEY WORDS. Key words are technically meaningful terms or short phrases that characterize a document and could be helpful in cataloging the document. Key words should be selected so that no security classification is required. Identifiers, such as equipment model designation, trade name, military project code name, geographic location, may be used as key words but will be followed by an indication of technical context.